


MEDICAL HOLE FINISH STAINLESS STEELS

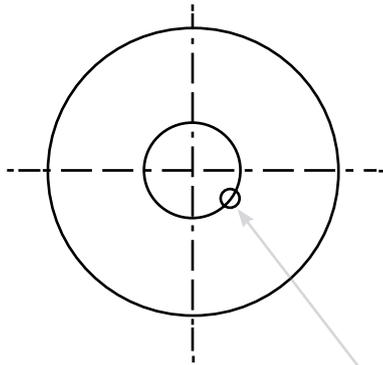

Cold worked	Transverse Rt	Longitudinal Ra
0 %	10 μ	
18 %	10 μ	0.25 μ
25 %	16 μ	
45 %	20 μ	

ID SURFACE CONDITION


Stainless steels

$\epsilon \approx 0\%$




x 62.5

$\epsilon \approx 18\%$

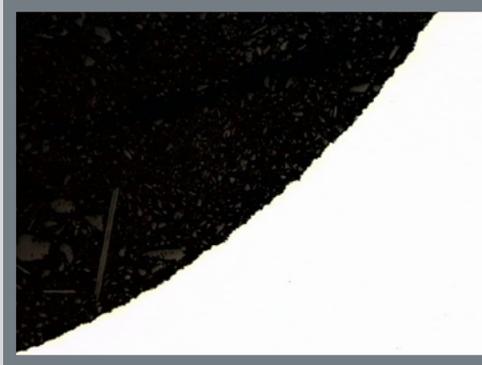

x 62.5

$\epsilon \approx 25\%$

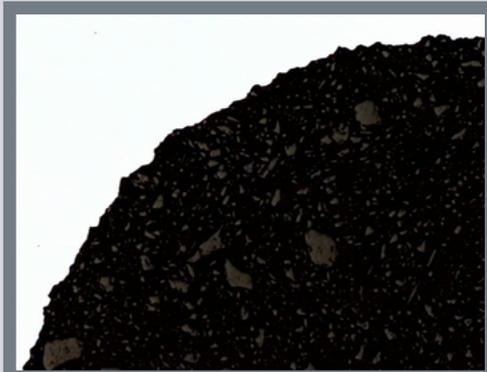

x 62.5

$\epsilon \approx 45\%$



x 62.5

Please contact our office for any additional information or documentation. Dimensional information and technical drawings in this document are for reference only. Some of the product characteristics indicated in this document may be modified at any time at the company's discretion. Our company is not responsible for the use of our products outside standards prescription and what our commercial documents are indicating.